


Miniflow[®]

Passive/ variable flow generator

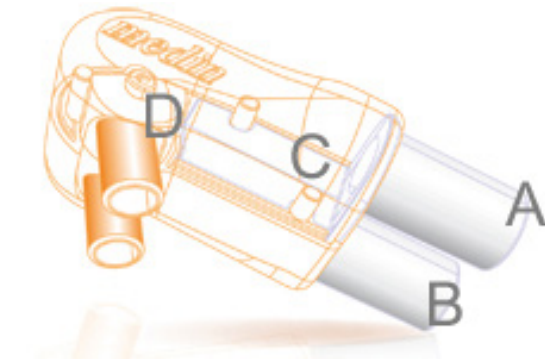

- A) Inspiration
- B) Expiration
- C) Separating wall
- D) Adjustable prong adapter

Parameters & sensors

CPAP pressures	0 to > 20mbar
Noise level	41 dB(A)
Volume reservoir ml	4 ml -constant flush
nCPAP pressure	> 4.5cm H ₂ O at 7 l/ml flow

Connectors

Inspiration	10mm OD/ 7,4 ID
Expiration	10mm OD/ 7,4 ID

Material	Terlux, TPE-S, Makrolon
----------	-------------------------

Consumables


Interfaces	Prongs and masks in various sizes
Bonnets	Color-coded and in different sizes available

Combinable devices	Hamilton T1, C1, MR1, C2, C3, C6, G5, S1, SLE6000 for more detailed informations, please read the Miniflow user manual.
--------------------	--

Standards

Classification	Class IIa
Certification	ISO 9001, ISO 13485 and 93/42/EEC certified production facility
Declaration	CE Marked product according to MDD 93/42/EEC



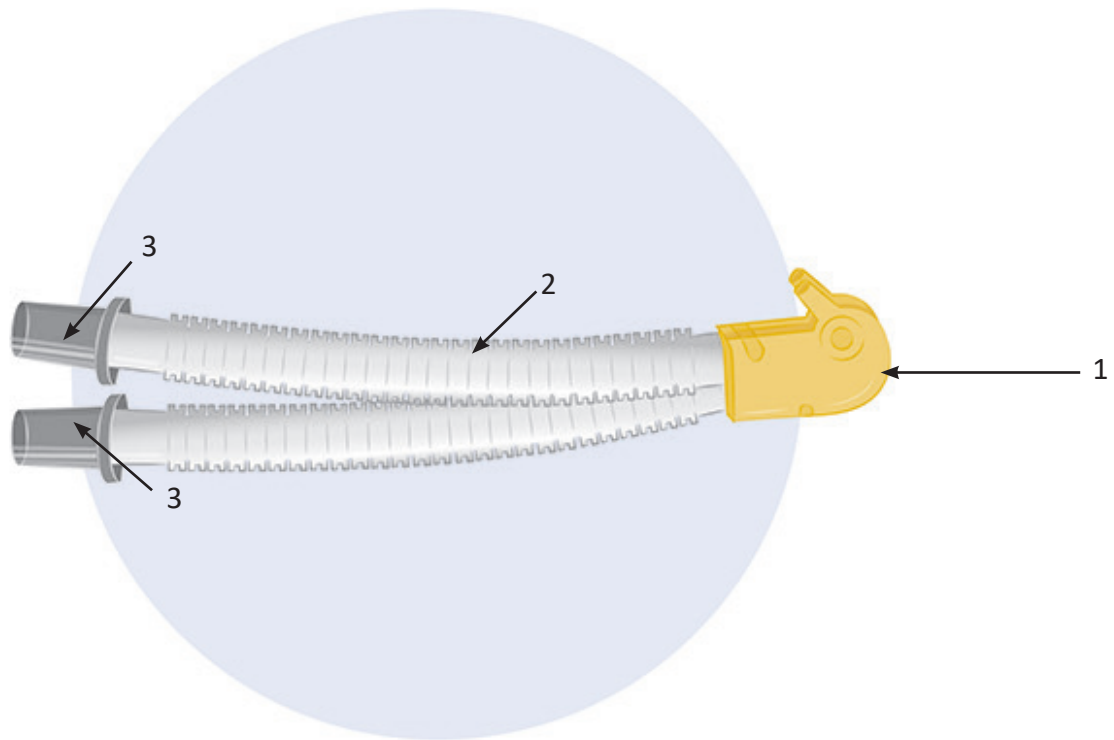

Material Medijet:

Terlux (1), TPE-S (2), Makrolon (3)

Material Measuring Tape:

ECF Paper

Material Minifoam:

Polyurethan-Etherfoam

Material Blister:

PE, Paper

Material Packaging:

Carton



medin Medical Innovations GmbH

Adam-Geisler-Straße 1

82140 Olching, Germany

+49 (0)8142 448 46 -0

info@medin-medical.com

www.medin-medical.com

CE0483

REV01
27.11.2019

Specifications are subject to change without notice. Some features are options. Not all features are available in all markets.
For all proprietary trademarks (®) and third-party trademarks (®) used by medin Medical Innovations GmbH see
www.medin-medical.com/trademarks. © 2019 medin Medical Innovations GmbH. All rights reserved.

Miniflow